



**CLIENT:** 0156  
**CONTACT:** Lab 1  
724 West Drive  
DeRidder, LA 70634

## CERTIFICATE OF ANALYSIS

**REPORT DATE:** 07Jul25  
**REPORT NUMBER:** RP156-02Jun25-1  
**QUOTE NUMBER:** QU-1064  
**PAGE:** 1 of 2


### SAMPLE IDENTIFICATION

**Sample Description:** Research Water 0.9% Benzyl Alcohol (Plastic Bottle)  
**Sample Lot Number:** Not provided  
**Date Received:** 02Jun25  
**PAL Sample Numbers:** 008122, 008123, 008124

**Test Requested:** Assay, % Benzyl Alcohol  
**Analysis date:** 12Jun25

Acceptance Criteria:  $0.9\% \pm 0.18$

Sample #	Sample Name	Result %	Pass/Fail
008122	Research water 0.9% Benzyl Alcohol	1.01	Pass

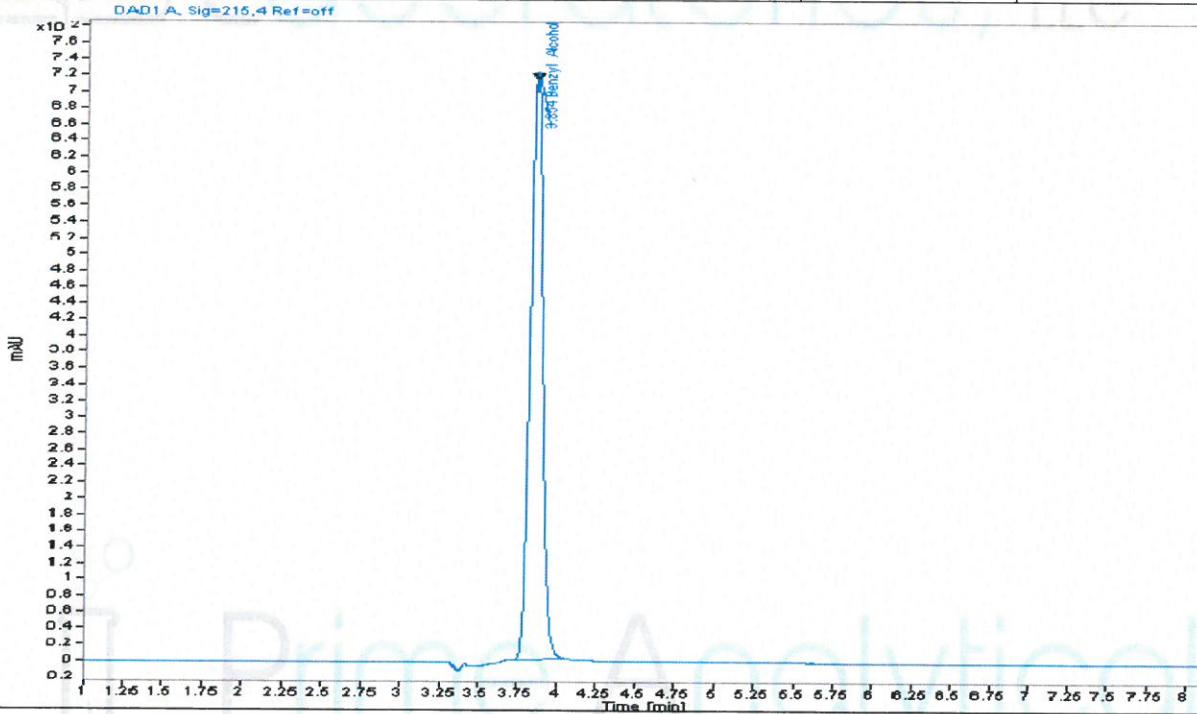

Percent Report Based on Area					
Name	RT [min]	Area	Height	RF	Amount [%]
Benzyl Alcohol	3.854	3635.7739	714.0215	0.00000	1.012

4055 Nelson Ave, Concord, CA 94520

Office (925) 235-1242

**CONFIDENTIAL**



## **CERTIFICATE OF ANALYSIS**

**CLIENT:** 0156  
**CONTACT:** Lab 1  
724 West Drive  
DeRidder, LA 70634

**REPORT DATE:** 07Jul25  
**REPORT NUMBER:** RP156-02Jun25-1  
**QUOTE NUMBER:** QU-1064  
**PAGE:** 2 of 2

**Test Requested:** MB-027, *USP <71> Sterility Testing*  
**Analysis date:** 20Jun25

## STERILITY RESULTS

STERILITY RESULTS			
Sample #	Sample Name	Acceptance Criteria	Results
008123	Research Water 0.9% Benzyl Alcohol	Pass/Fail	Pass

**Test Requested:** MB-026, USP <85> Kinetic Turbidimetric Assay (BET) Using the Pyros Kinetix Flex  
**Analysis Date:** 03Jul25

## ENDOTOXIN RESULTS      Acceptance Criteria: < 0.5 EU/mL

Sample #		Sample Name	Results	Pass/Fail/Invalid
008124	Research Water 0.9% Benzyl Alcohol	< 0.1 EU/mL	Pass	

Note: Result(s) reported above relate only to the sample(s) tested.

Prepared by/date: John Doe 07Jul25 Approved by/date:  
Laboratory Services

Praj 05Aug25  
Quality Assurance